

**CAUTION**


TO PROVIDE CONTINUED PROTECTION AGAINST THE RISK OF ELECTRIC SHOCK, CUSTOMER'S POWER SUPPLY MUST BE PROPERLY GROUNDIED.

NOTE: GROUNDING SCREW TO HAVE A GREEN COLORED SLOTTED AND/OR HEX HEAD NO SUBSTITUTES. USE #1005

NOTE: THE SURFACE OF THE INSULATED WIRES MARKED (X) TO BE COLORED GREEN, WITH OR WITHOUT ONE OR MORE YELLOW STRIPES.

**WIRING NOTE**

ALL WIRES #14 AWG, TYPE SEW/SF2 MINIMUM UNLESS OTHERWISE NOTED

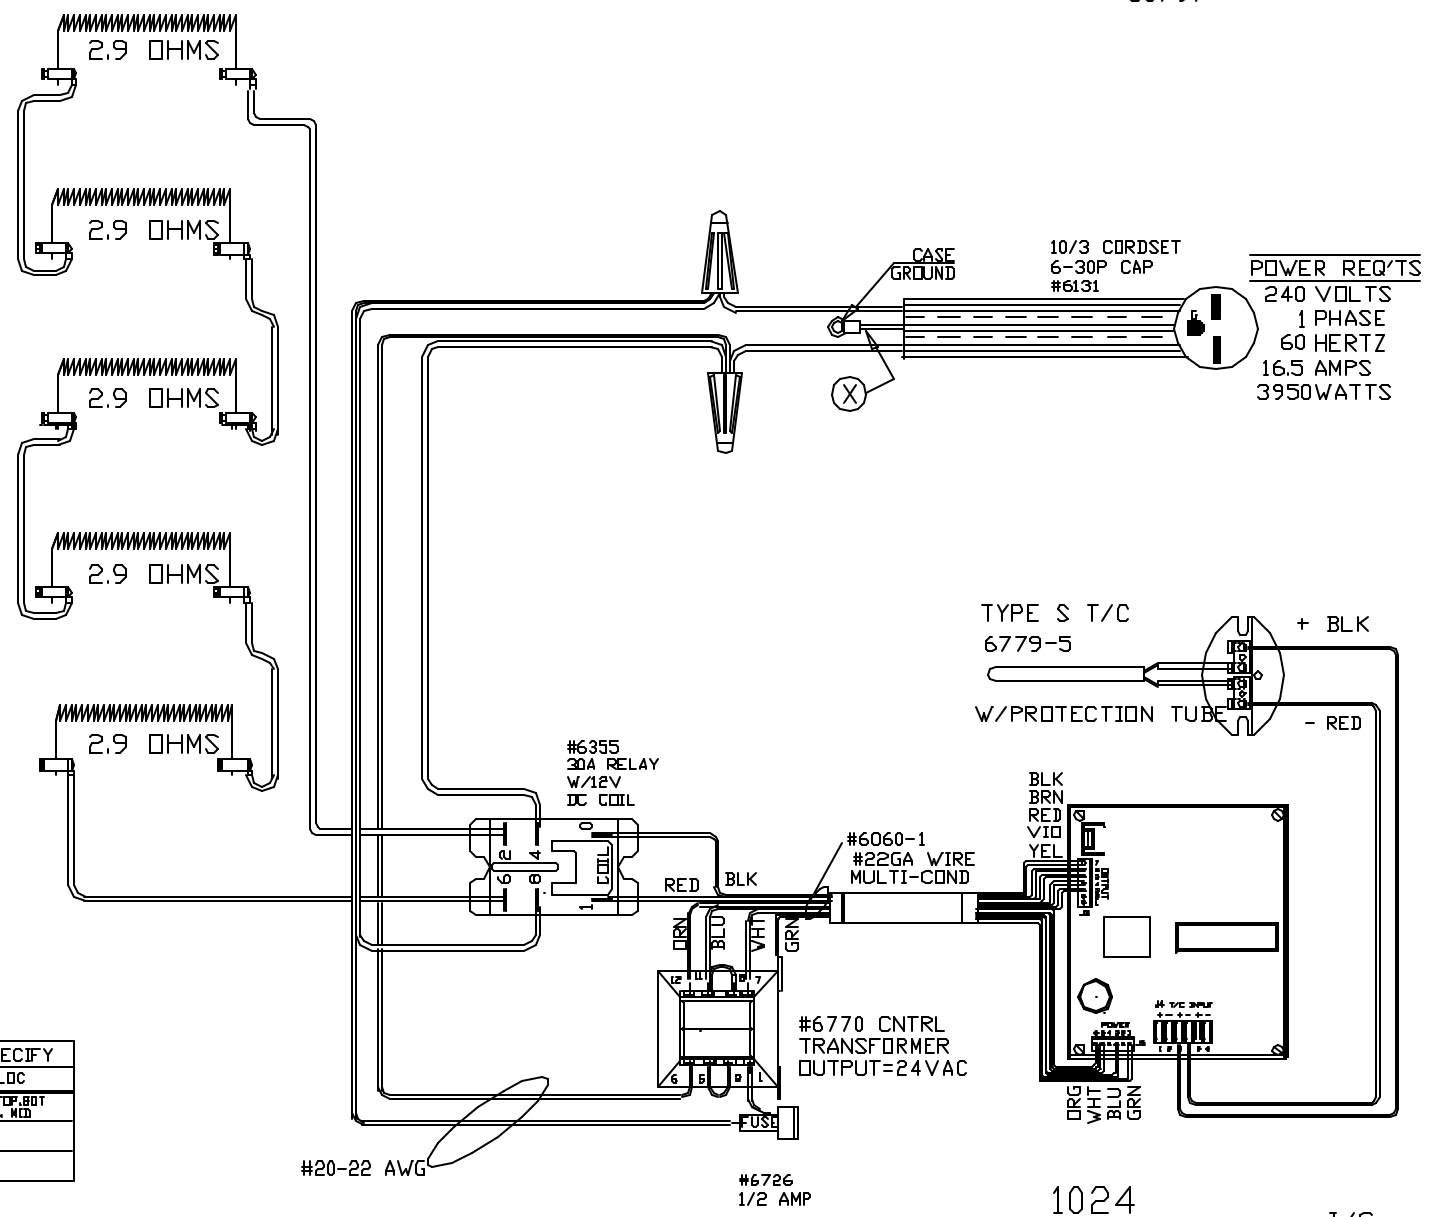

**POWER REQ'TS**  
 240 VOLTS  
 1 PHASE  
 60 HERTZ  
 16.5 AMPS  
 3950WATTS

| TO RE-ORDER ELEMENTS, SPECIFY |     |               |
|-------------------------------|-----|---------------|
| DESCRIPTION                   | QTY | LOC           |
| ELS0797TBM                    | 3   | TOP BOT & MED |
|                               |     |               |
|                               |     |               |

1024  
 SENTRY 2.0 I/C  
 2350° F

| REV | DATE   | BY  | DESCRIPTION |
|-----|--------|-----|-------------|
| -   | 2/6/02 | RLG |             |
|     |        |     |             |
|     |        |     |             |

SWITCH BOX ASSY- 42026  
 PARAGON INDUSTRIES  
 2011 SOUTH TOWN EAST BLVD  
 MESQUITE, TEXAS 75149

**WIRING DIAGRAM**  
 240V 1 PHASE 60HZ 3950WATTS

PART NO S0797  
 CRUCIBLE 13.5X14.25

REV A  
 FILE